


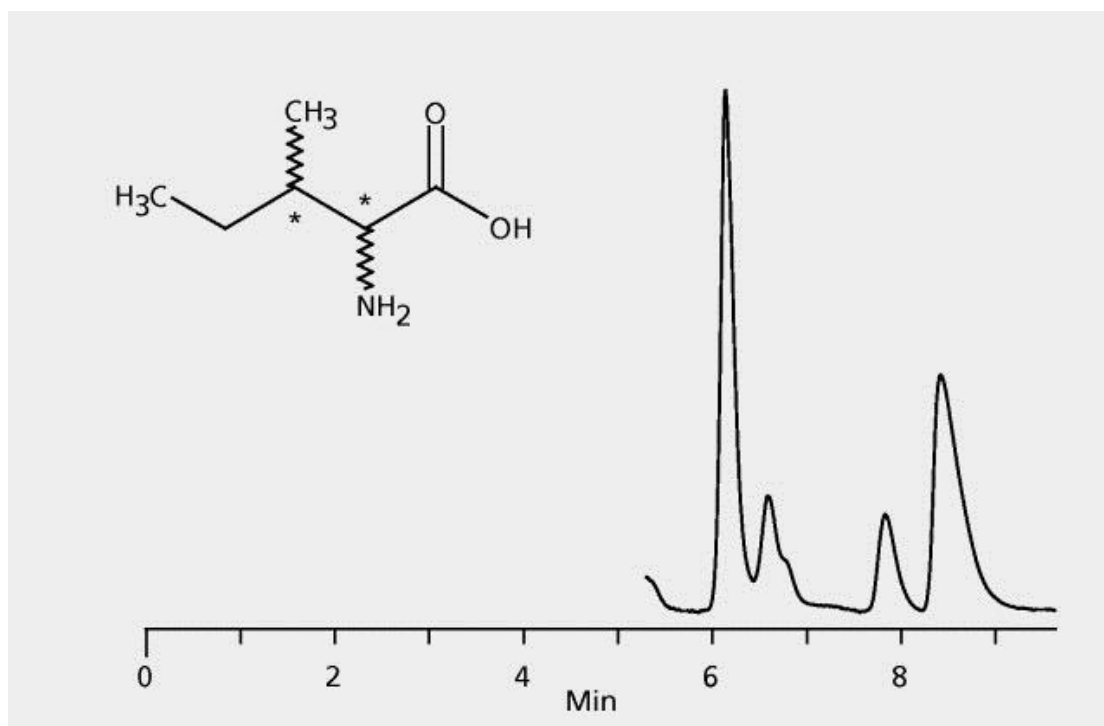

test parameters	column: CHIROBIOTIC R, 25 cm x 4.6 mm I.D., 5 µm particles (13024AST)
	mobile phase: (A) water; (B) methanol; (40:60, A:B)
	flow rate: 0.6 mL/min
	column temp.: 25 °C
	detector: UV, 210 nm
	injection: 10 µL
	sample: 1 mg/mL in methanol