


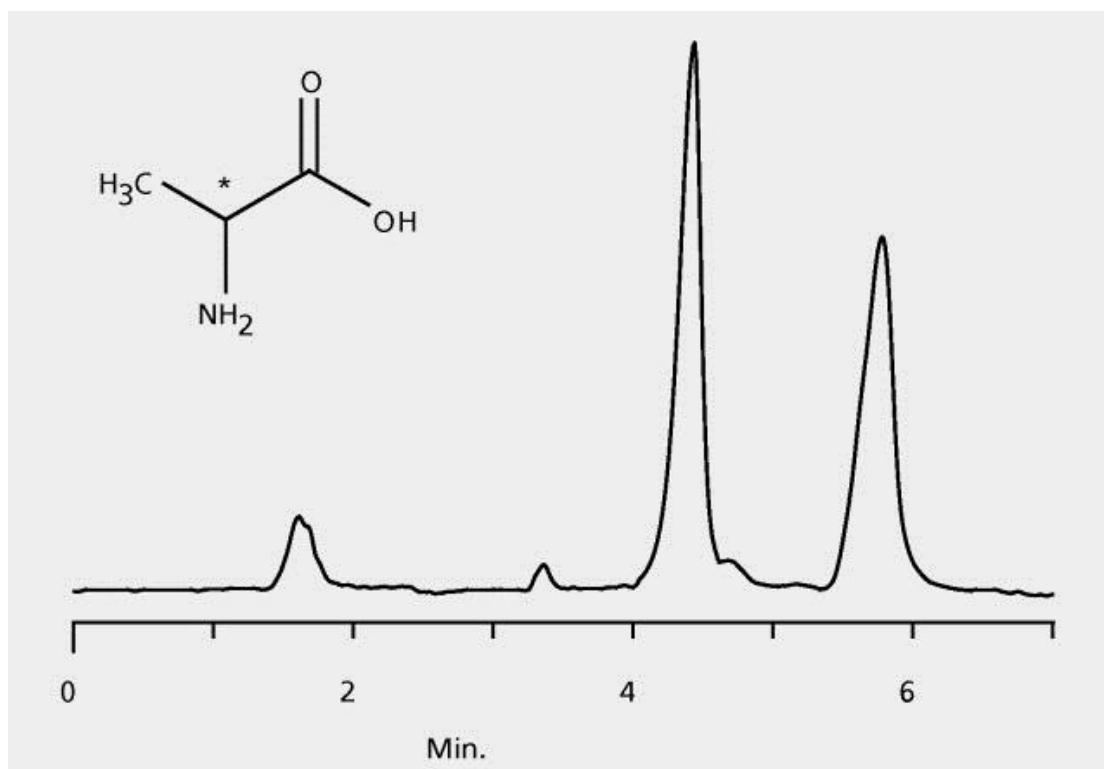

test parameters	column: CHIROBIOTIC TAG, 25 cm x 4.6 mm I.D., 5 µm particles (14024AST)
	mobile phase: (A) water; (B) acetonitrile; (50:50, A:B)
	flow rate: 0.8 mL/min
	column temp.: 25 °C
	detector: UV, 210 nm
	injection: 2 µL
	sample: 5 mg/mL in methanol