


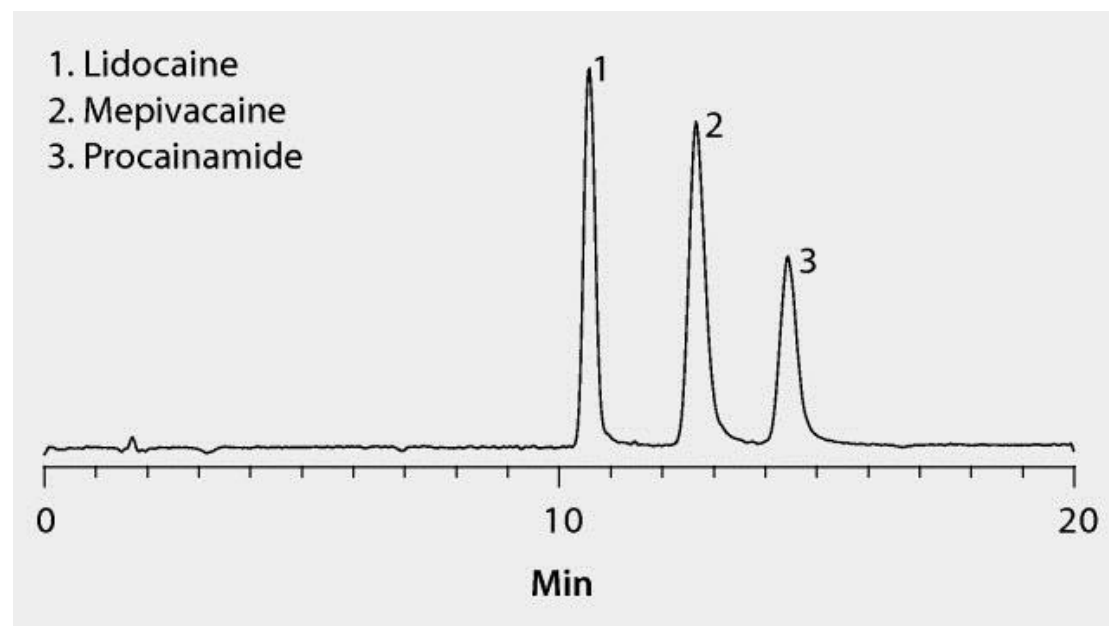

test parameters	column: Ascentis Express F5, 10 cm x 4.6 mm I.D., 2.7 µm particles (53590-U)
	mobile phase: (A) 10 mM ammonium acetate, pH 4.0 with acetic acid; (B) acetonitrile; (20:80, A:B)
	flow rate: 1.0 mL/min
	pressure: 160 bar
	column temp.: 35 °C
	detector: MS, ESI(+), SIR, m/z 235, 236, 247
	injection: 2 µL