


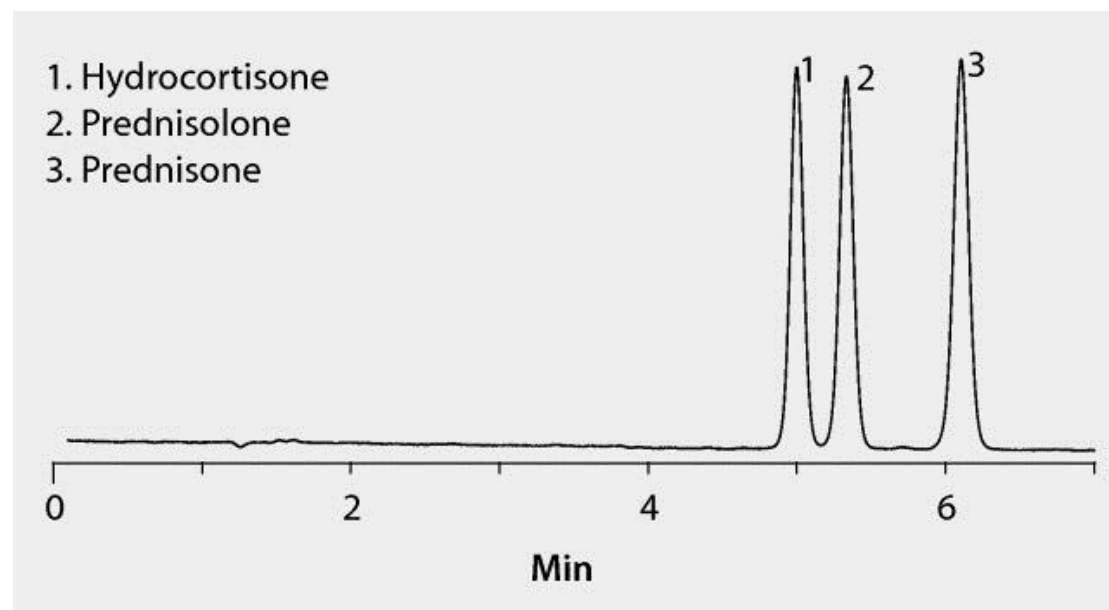

test parameters	column: Ascentis Express F5, 15 cm x 4.6 mm I.D., 2.7 µm particles (53591-U)
	mobile phase: (A) water; (B) methanol; (50:50, A:B)
	flow rate: 0.8 mL/min
	pressure: 165 bar
	column temp.: 35 °C
	detector: UV, 240 nm
	injection: 5 µL
	sample: 10 µg/mL of each in 90: 10, water: methanol