


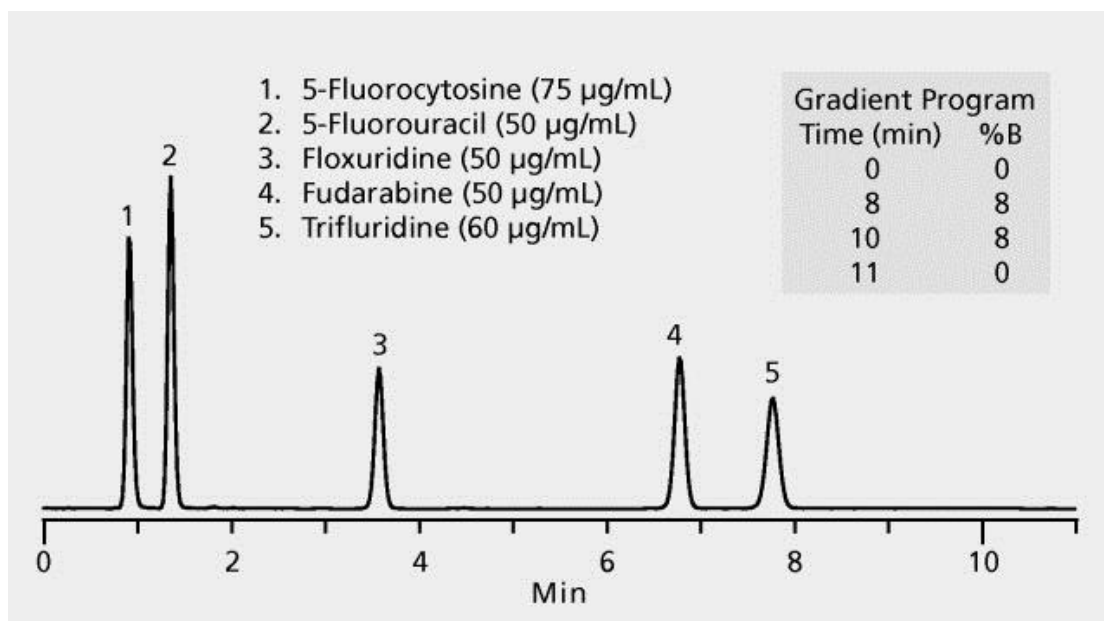

test parameters	column: Ascentis RP-Amide, 5 cm × 4.6 mm I.D., 5 µm particles (565323-U)
	mobile phase: (A) water with 0.1% ammonium formate (pH 3.04 with formic acid), (B) acetonitrile
	flow rate: 1.0 mL/min
	column temp.: 30 °C
	detector: UV, 260 nm
	injection: 5 µL
	sample: as indicated in mobile phase A