


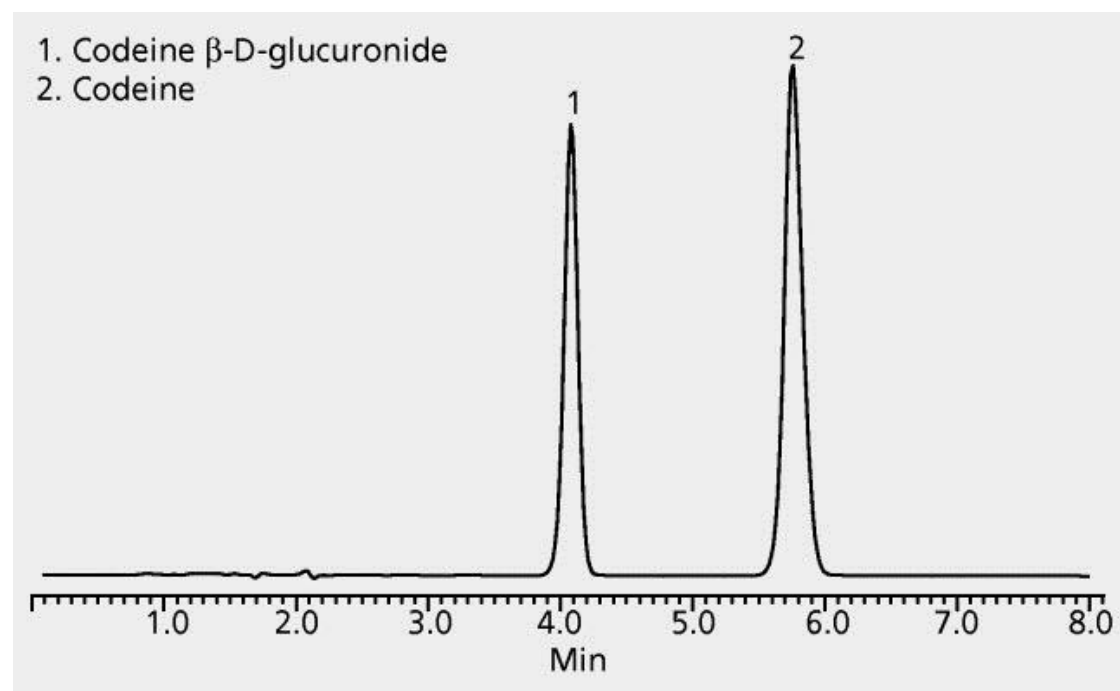

test parameters	column: Ascentis RP-Amide 15 cm x 4.6 mm I.D., 5 μ m particles (565324-U)
	mobile phase: (A) 10 mM monobasic potassium phosphate (pH 3.0 with phosphoric acid); (B) acetonitrile; (90:10, A:B)
	flow rate: 1 mL/min
	column temp.: 35 $^{\circ}$ C
	detector: UV, 220 nm
	injection: 10 μ L
	sample: 50 μ g/mL each in mobile phase