


1. Oxycodone
2. Noroxycodone
3. Cocaine
4. Cocaethylene

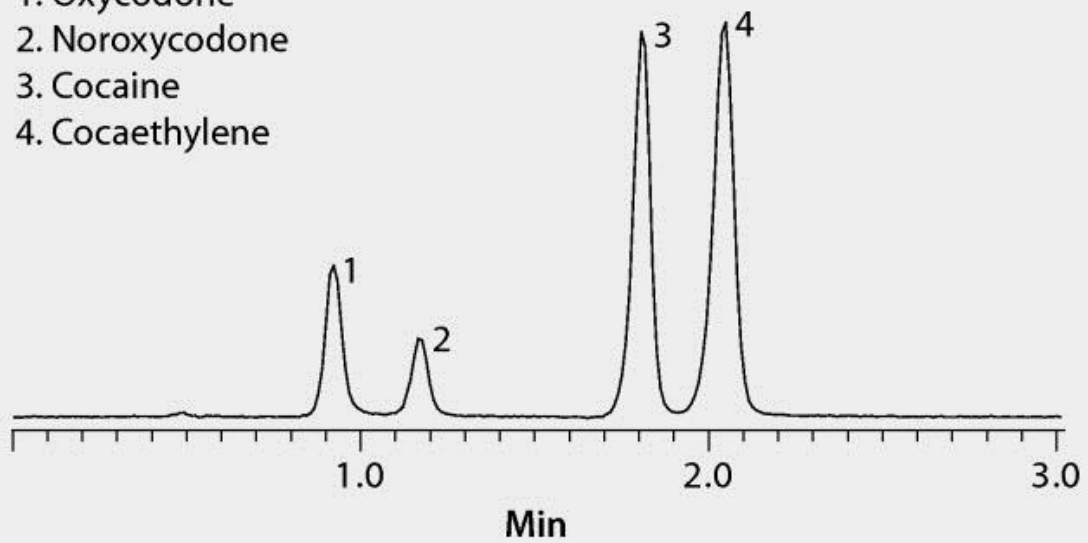

test parameters	column: Discovery HS F5, 5 cm x 2.1 mm I.D., 3 μ m particles (567500-U)
	mobile phase: (A) 10 mM ammonium formate in water, pH 6.8; (B) 10mM ammonium formate in acetonitrile, pH 6.8; (10:90, A:B)
	flow rate: 0.3 mL/min
	column temp.: 35 $^{\circ}$ C
	detector: ESI(+)
	injection: 2 μ L
	sample: 200 ng/mL in 25:75, water:acetonitrile