


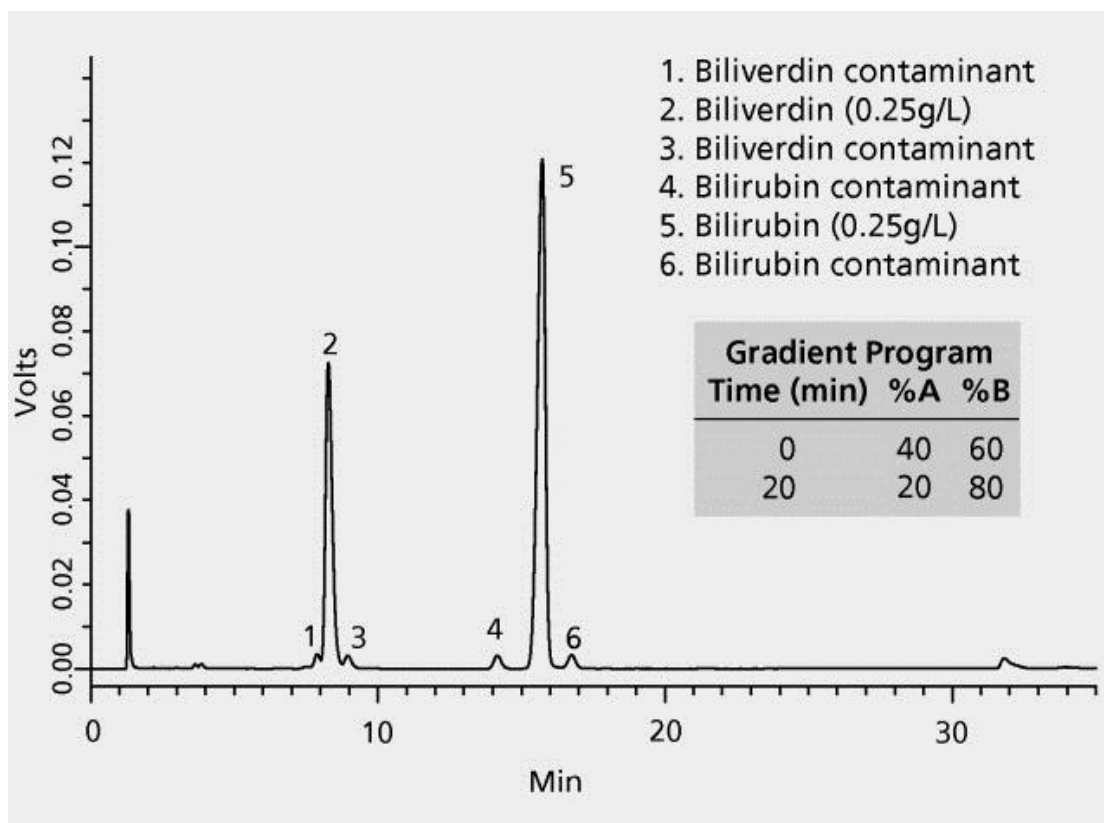

test parameters	column: Discovery C18, 10 cm × 2.1 mm I.D., 5 µm particles (569220-U)
	mobile phase: (A) 10 mM ammonium acetate (pH unadjusted) (B) 90:10, methanol:(100 mM ammonium acetate)
	flow rate: 0.2 mL/min
	column temp.: ambient
	detector: UV, 405 nm
	injection: 1 µL
	sample: as indicated (in 50% MeOH, 1% NH ₄ OH)