


1. Lasalocid A (1 µg/mL); m/z 589.5
2. Monensin (10 µg/mL); m/z 669.6
3. Salinomycin SV (10 µg/mL); m/z 749.5
4. Narasin (3 µg/mL); m/z 763.5

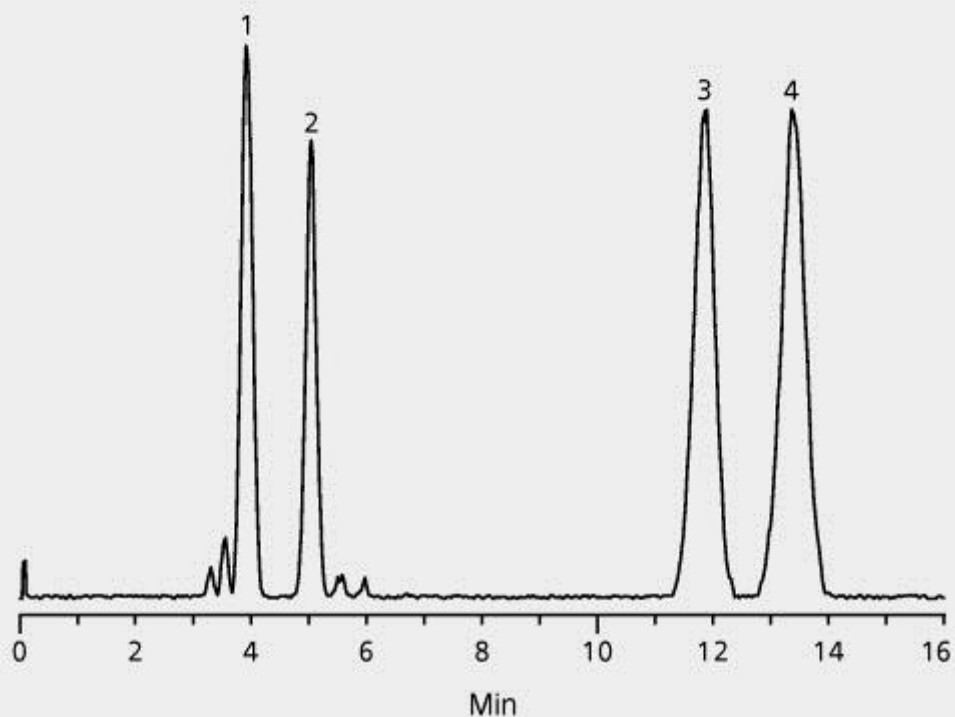

test parameters	column: Discovery HS C18, 5 cm × 2.1 mm I.D., 3 µm particles (569253-U) mobile phase: (A) (50 mM acetic acid/ammonium hydroxide, pH 6.0]: (B) methanol; (20:80, A:B): flow rate: 0.2 mL/min
	column temp.: 22 °C
	detector: ESI (+), full scan
	injection: 2 µL
	sample: as indicated in 50:50 water:methanol