

Cyclodextrins

Column: YMC-Pack ODS-A
(150 x 4.6 mm)

Eluent: A = H₂O


B = Methanol

Gradient: 2% B (0-5 min), 2-30% B (5-15 min, linear), 30-100% B (15-20 min, linear), 100% B (20-30 min)

Flow: 1.0 ml/min

Detection: Evaporative Mass Analyser

Temperature: 30 °C

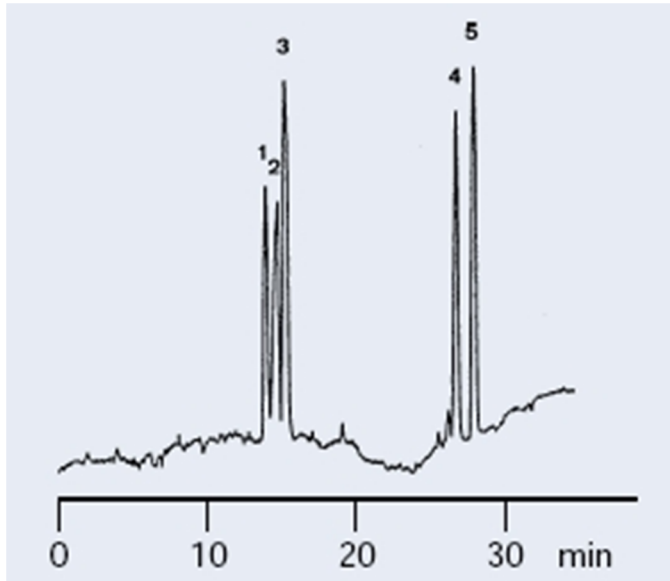

1: γ -Cyclodextrin

2: α -Cyclodextrin

3: β -Cyclodextrin

4: o-Dimethyl- β -Cyclodextrin

5: o-Trimethyl- β -Cyclodextrin